SonoSite X–Porte AC Cord Retainer Installation Instructions
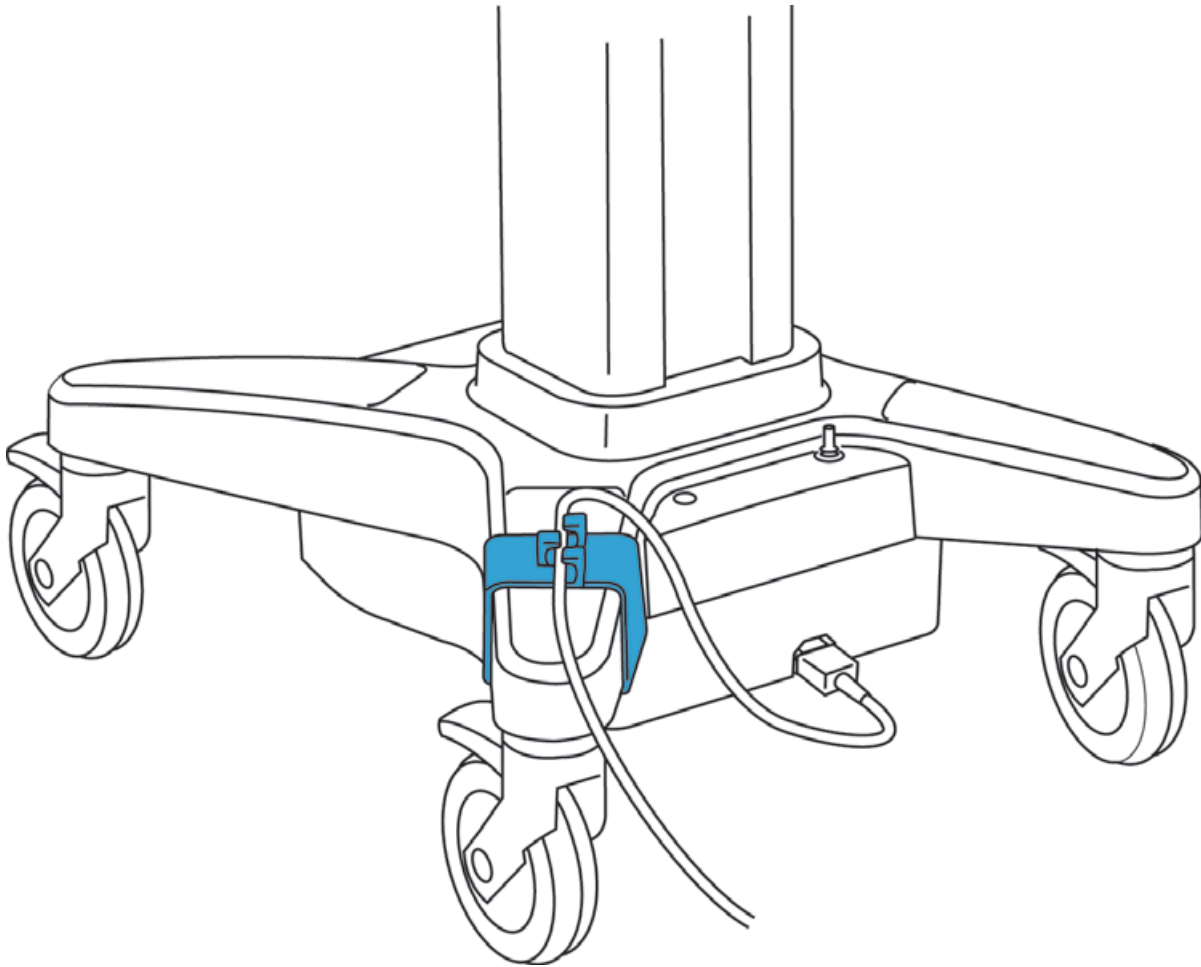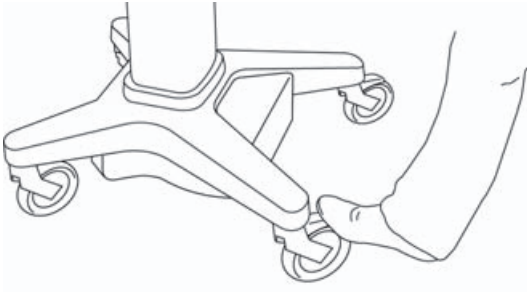
Contents
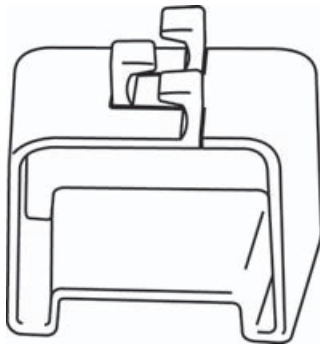
AC Cord Retainer (1)
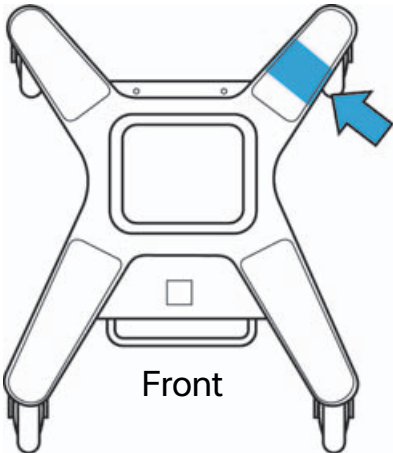
Preparing the stand

STEP 1

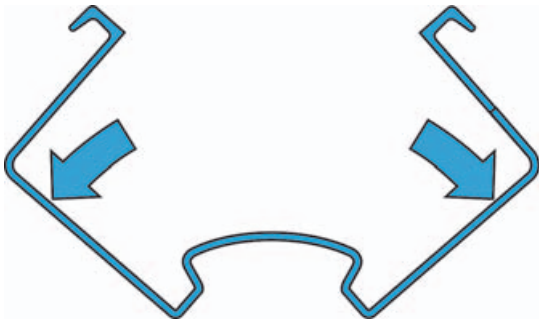Press down the lever on two or more wheels.

Attaching the AC cord retainer

STEP 2

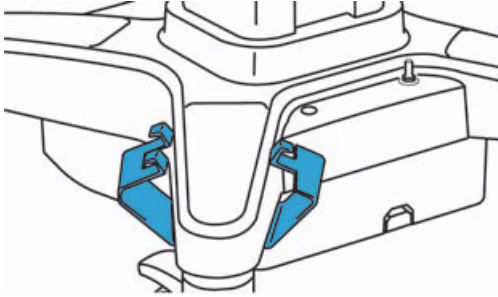Find the right-rear leg of the stand.

Front

STEP 3

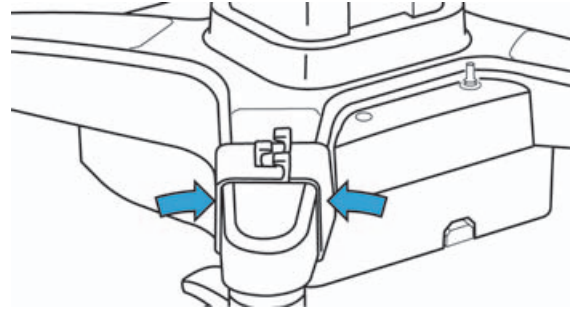Spread the AC Cord Retainer apart.

STEP 4

Wrap the AC Cord Retainer around the right-rear leg of the stand.
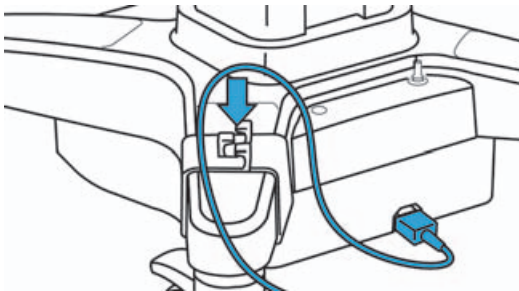

STEP 5

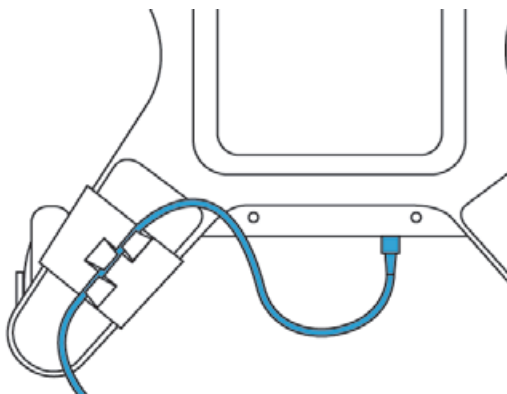Close the AC Cord Retainer around the stand leg.

STEP 6

Pass the AC power cord through the hooks in the AC Cord Retainer. The arrangement of the cord may differ, depending on your configuration. See the examples below.
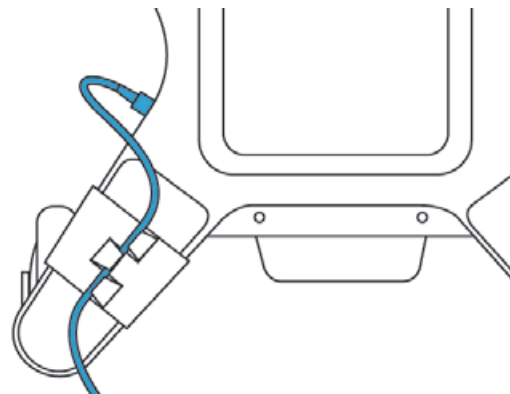

EXAMPLE A

AC power cord attached to the stand base.

EXAMPLE B

AC power cord attached to a PowerPark stand module.

For cleaning, storage, and disposal

▸ For cleaning instructions, see the system user guide.

▸ Storage requirements: Temperature: –35°C to 65°C; Humidity: 15% to 95%; Atmospheric pressure: 500 hPa to 1060 hPa.

▸ To dispose of the AC cord retainer, contact FUJIFILM SonoSite, or your authorized representative.

Caution	Federal (United States) law restricts this device to sale by or on the order of a physician.

X-Porte, SonoSite, and the SonoSite logo are trademarks or registered trademarks of FUJIFILM SonoSite, Inc. in various jurisdictions. Value from Innovation is a trademark of FUJIFILM Holdings America Corporation.

All other trademarks are the property of their respective owners.

Publication Date: November 2016

Manufacturer	**EC Authorized Representative**	**Australia Sponsor**	
FUJIFILM SonoSite, Inc.	Emergo Europe	FUJIFILM SonoSite Australasia Pty Ltd	
21919 30th Drive SE	Molenstraat 15		
Bothell, WA 98021 USA	2513 BH, The Hague	114 Old Pittwater Road	CE
T: 1-888-482-9449 or 1-425-951-1200	The Netherlands	BROOKVALE, NSW, 2100	
F: 1-425-951-1201		Australia	

P22734-01

4